


**FIG. 1**

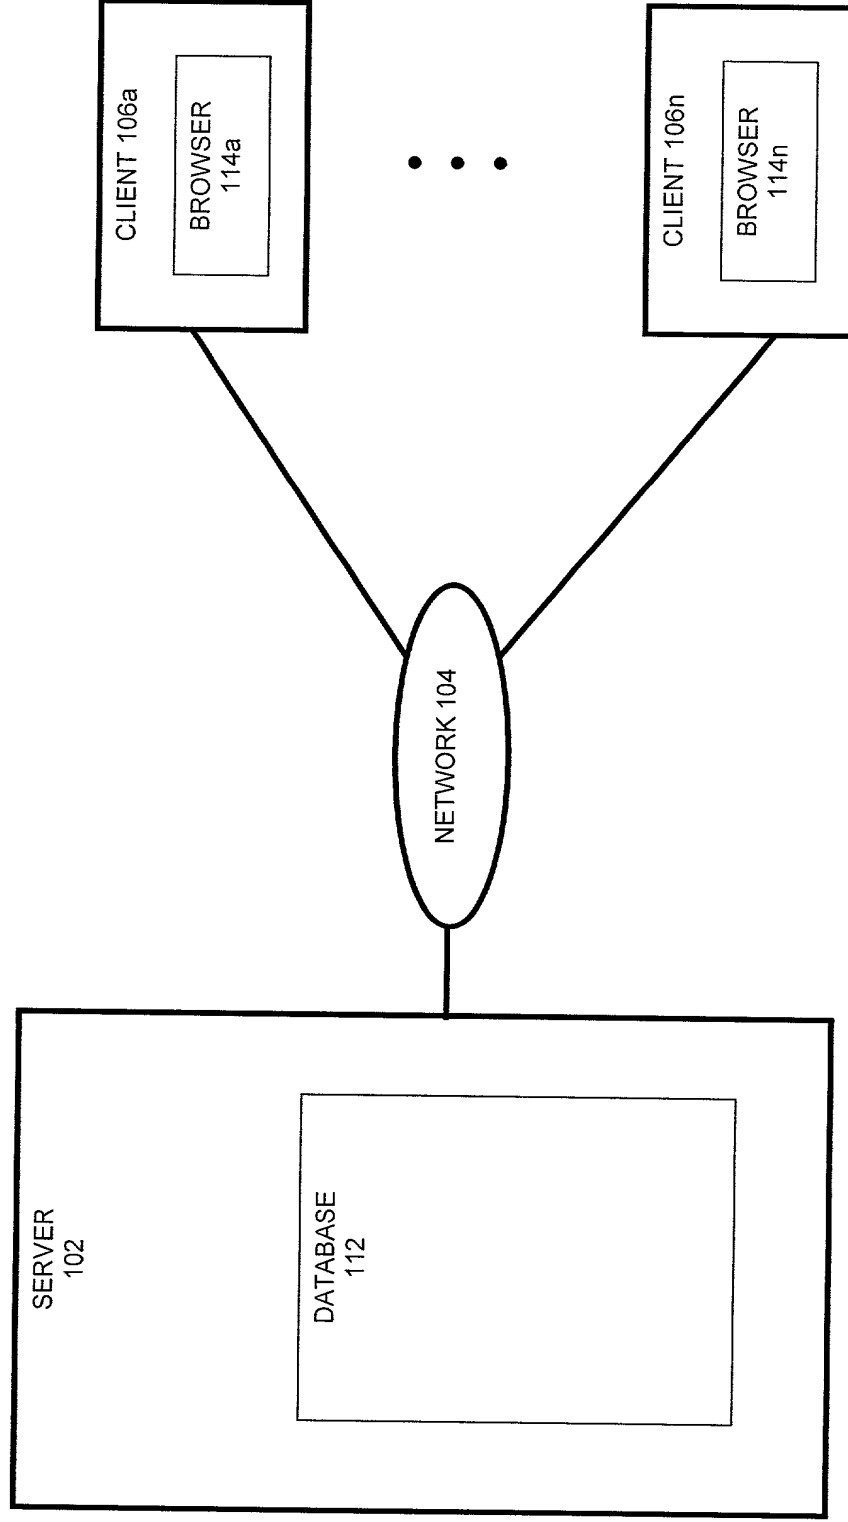

**FIG. 2**

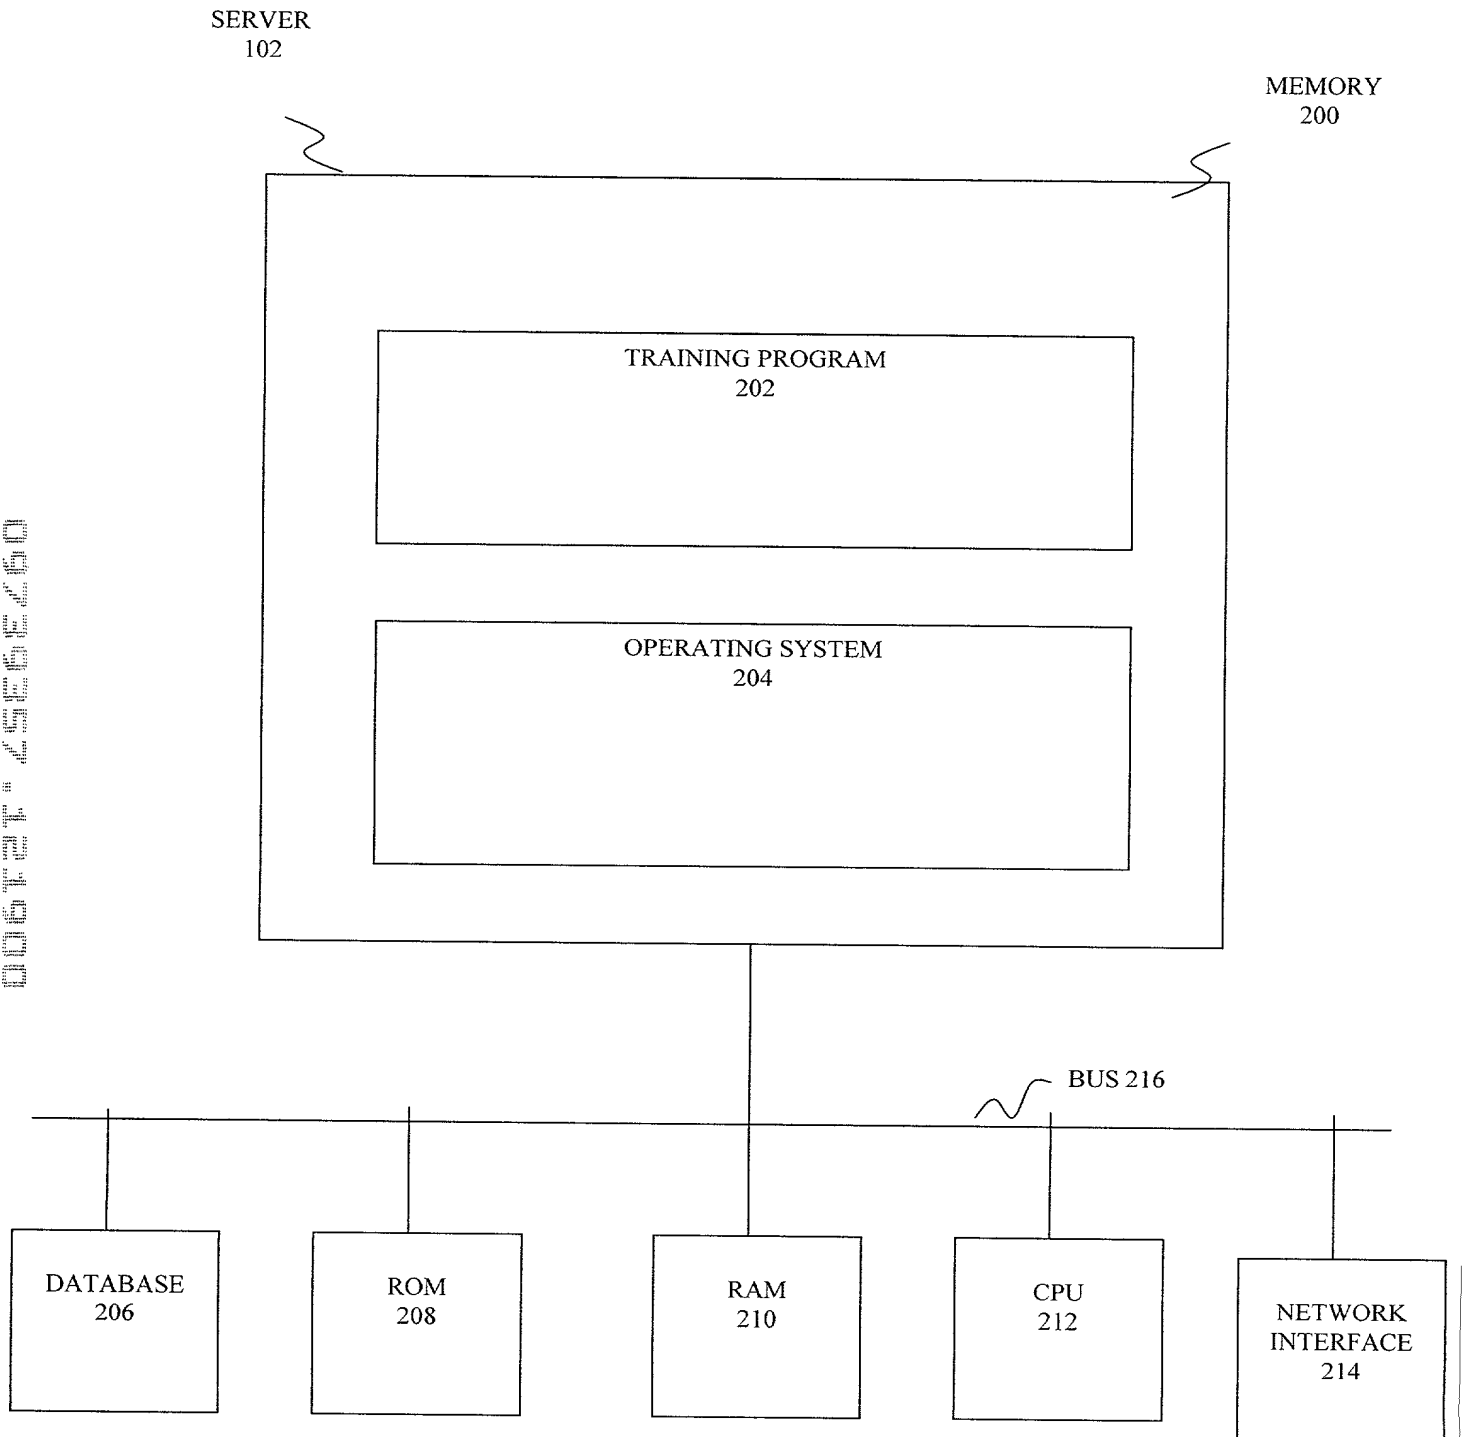


FIG. 3

USER COMPUTER 106

MEMORY 302

BROWSER PROGRAM  
304

OPERATING SYSTEM  
306

BUS 318

ROM  
308


RAM  
310

DISPLAY  
INTERFACE  
312

CPU  
314

NETWORK  
INTERFACE  
316

20160624 16:56:50

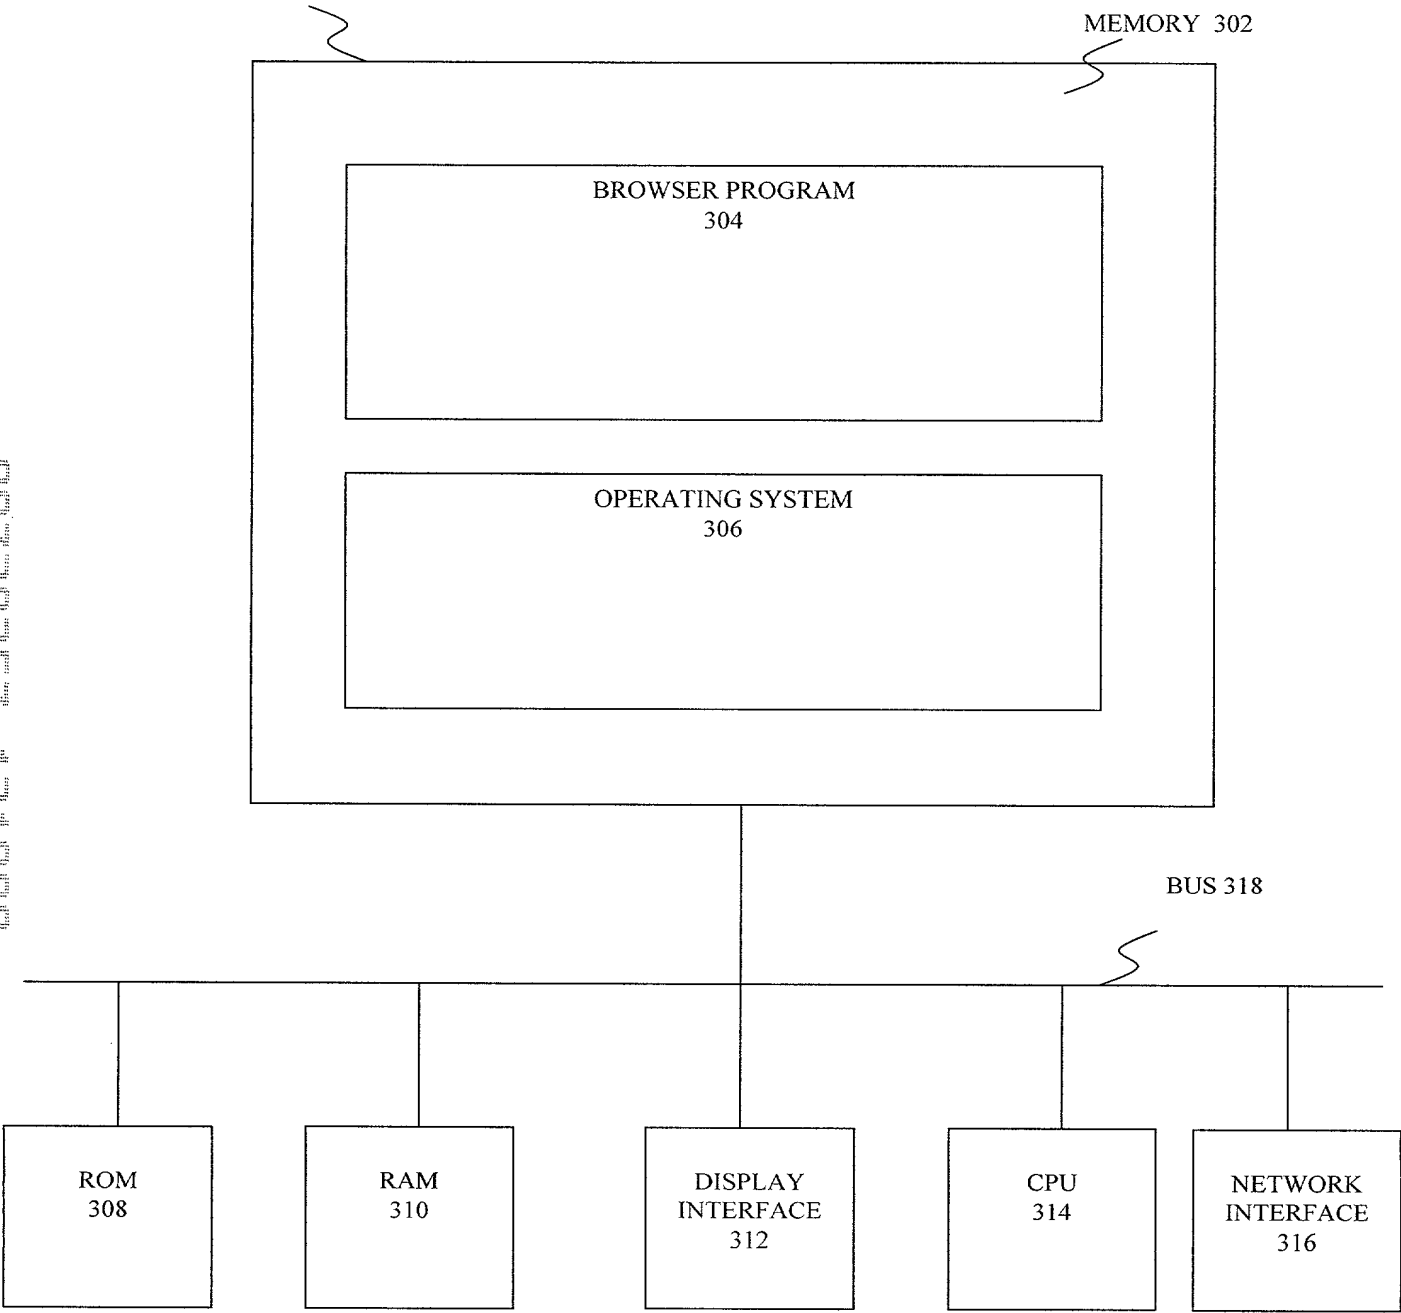

**FIG. 4**


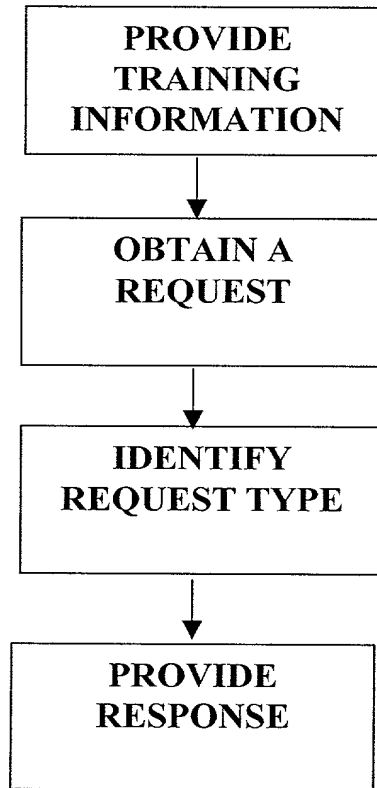


FIG. 5

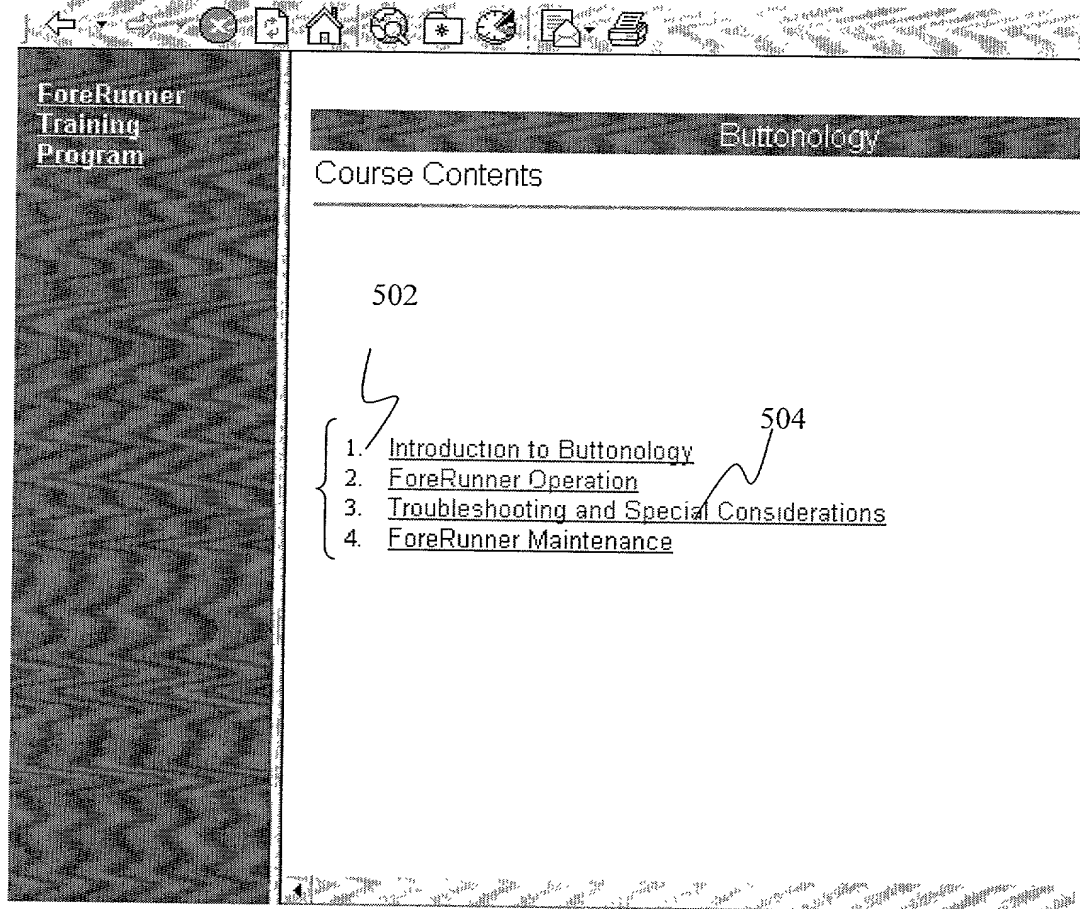

# FIG. 6

600

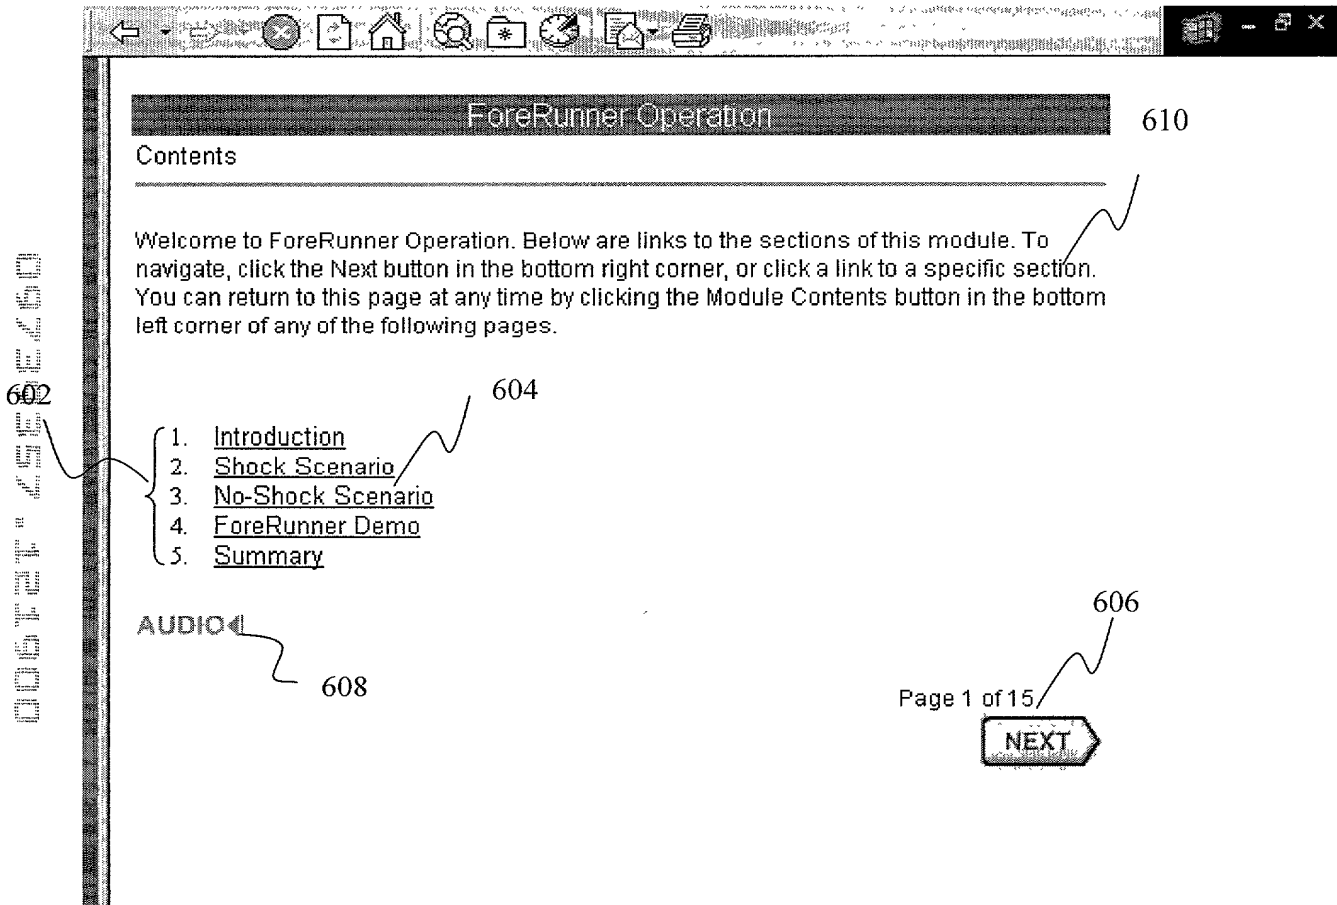


FIG. 7

700

006121/3668/60


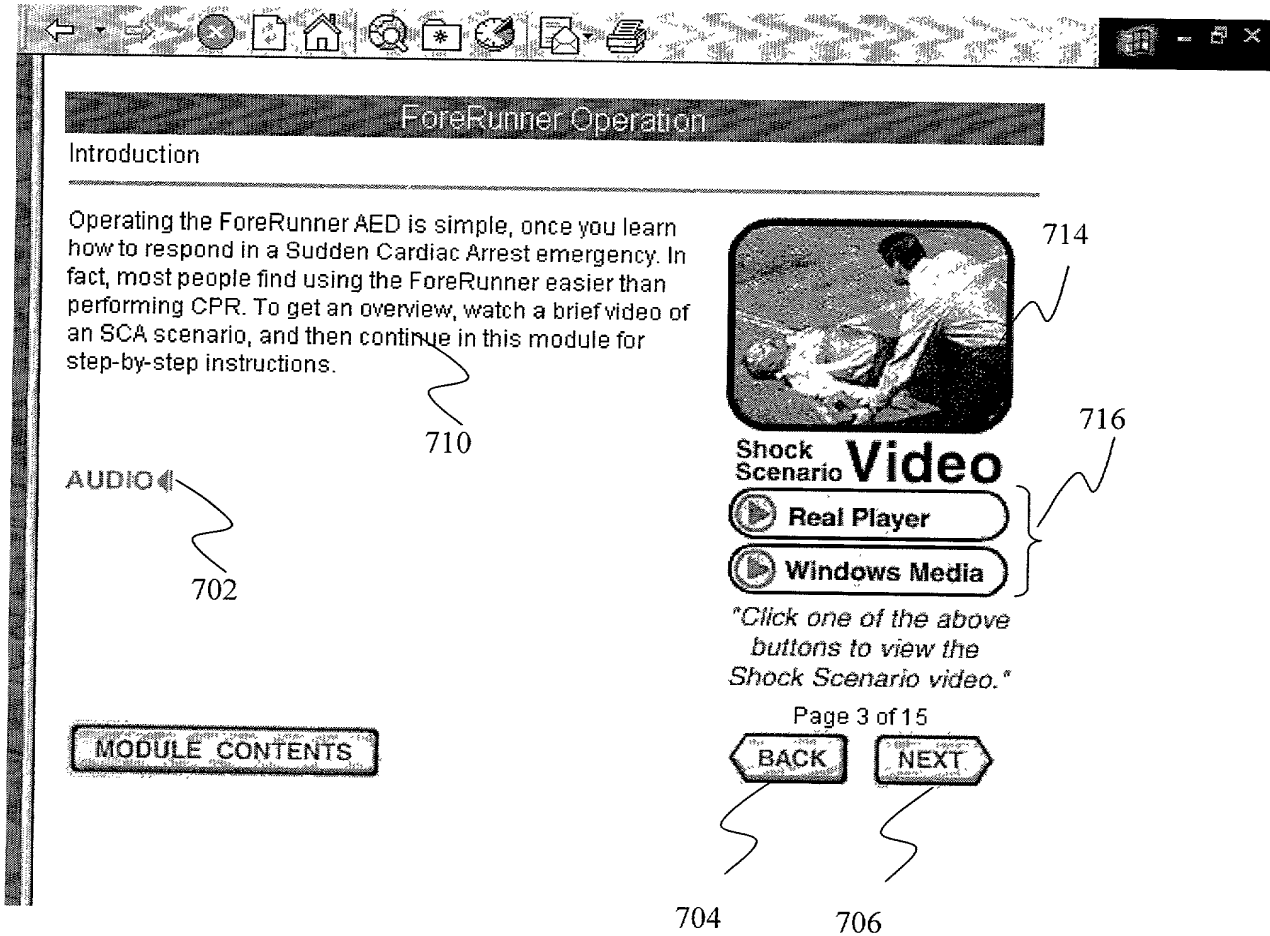


FIG. 8


800



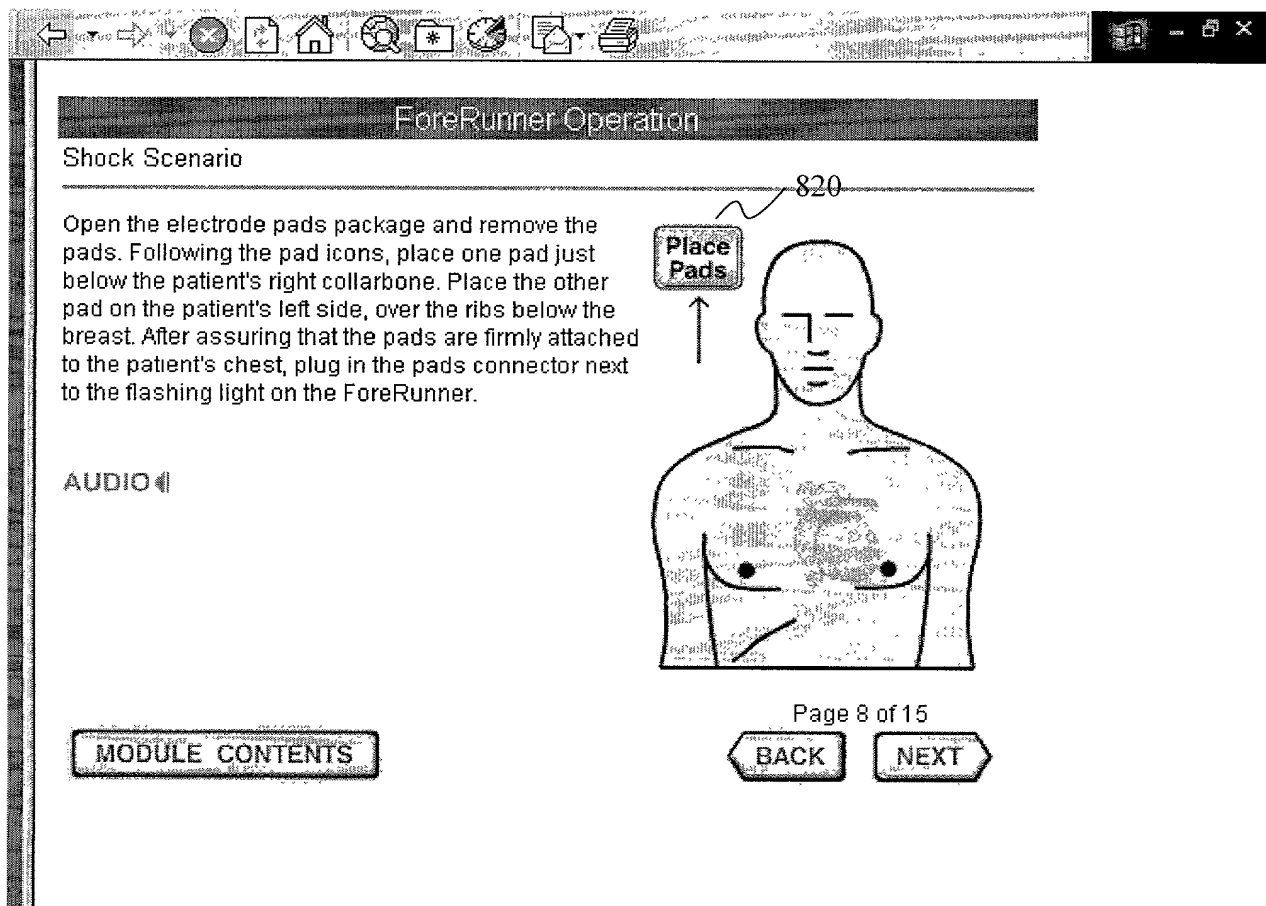

# FIG. 9

900

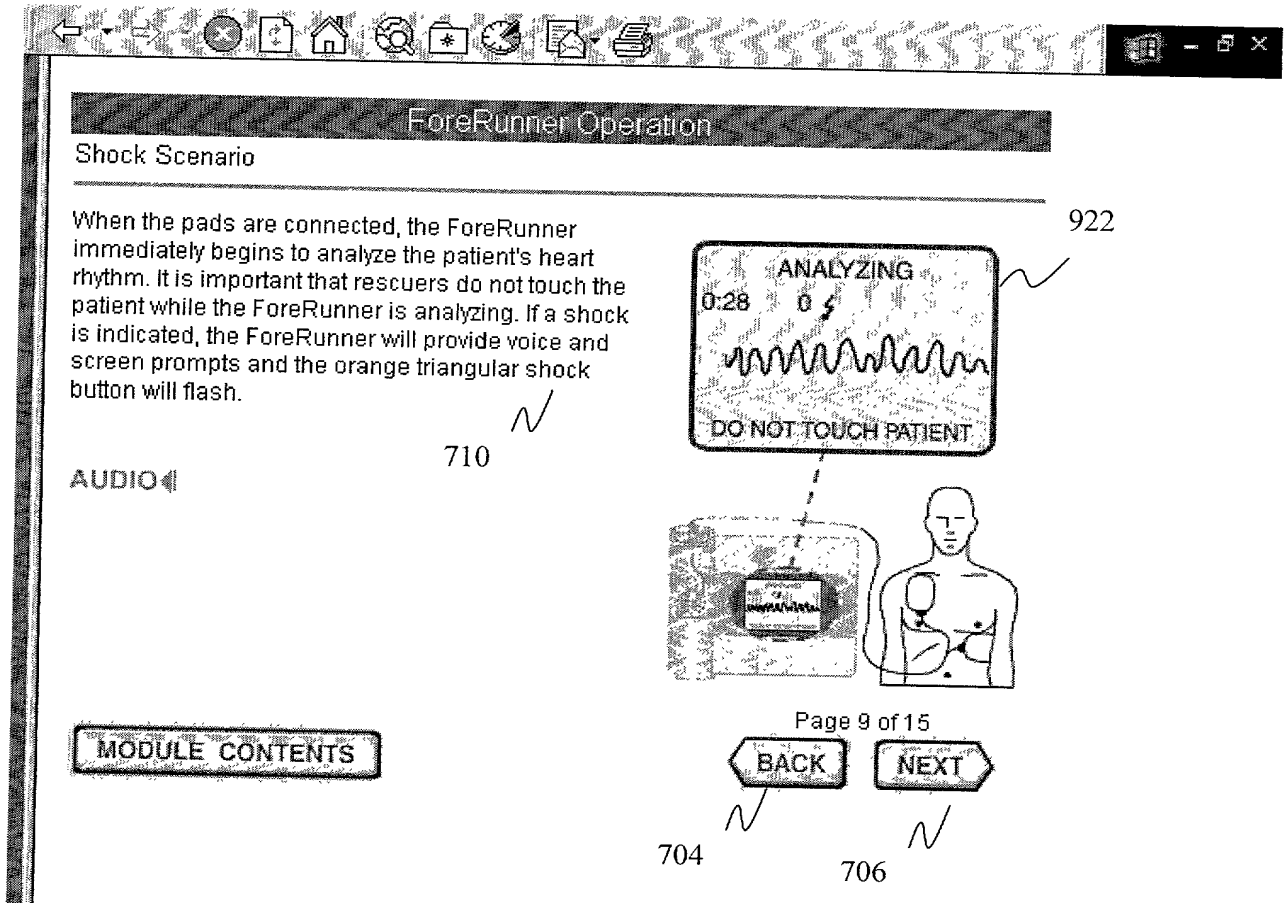

# FIG. 10

1000


005121 4566250

ForeRunner Operation

Shock Scenario

Before delivering the shock, it is important that the ForeRunner operator visually and verbally clears the patient. The ForeRunner operator should shout, "I'm clear," "you're clear," or simply "clear." Visually check to be certain that no one is touching the patient.

710




1518

After making sure everyone is clear of the patient, press the orange button to deliver the shock.

1024

AUDIO



MODULE CONTENTS

Page 10 of 15

BACK

NEXT

# FIG. 11

1100

